


In the US, Philips will not return to the sale of hospital ventilation products, and certain out-of-hospital respiratory care products.

19 sleep and respiratory products are discontinued in the US



● Sales discontinuation
● End of Service

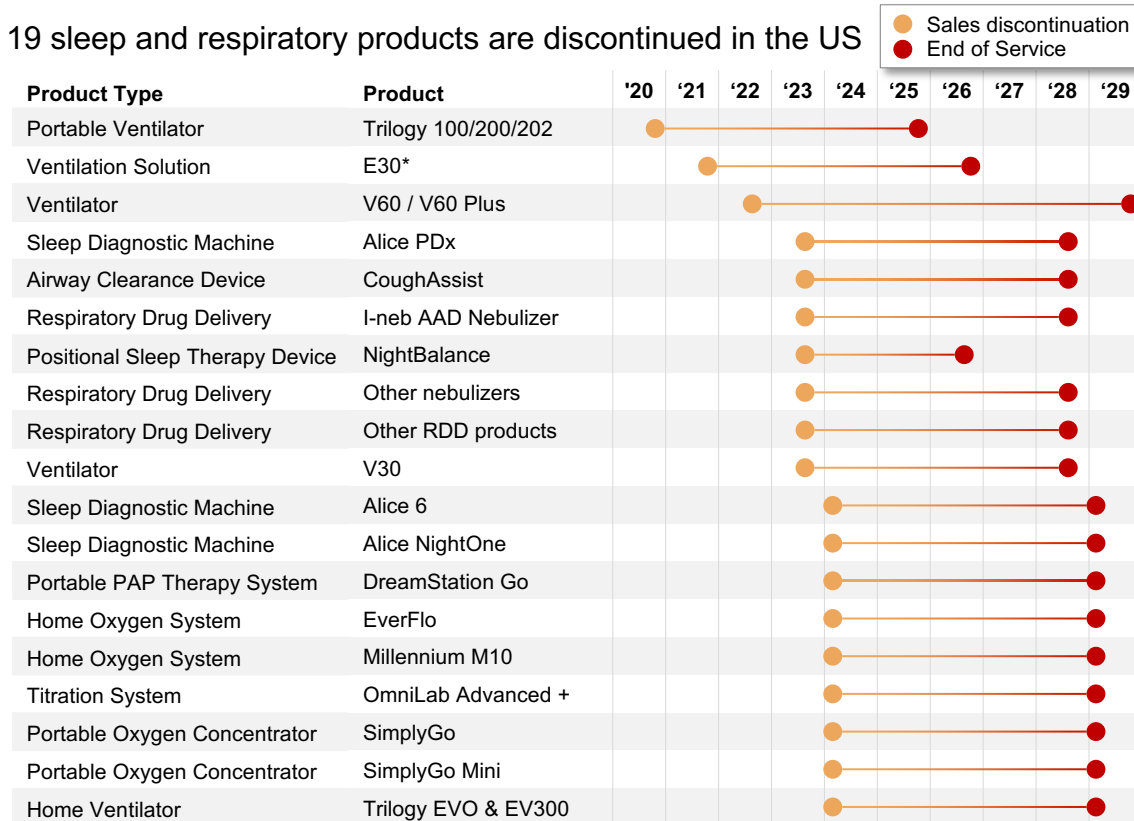

- Philips agrees with US FDA on the terms of a consent decree on Jan 29, 2024.



- Philips would halt sales of all of its breathing machines in the US, until the relevant requirements of the consent decree are met.



“When we have the consent decree, then the timeline will be clarified, but it normally takes five to seven years.”

Roy Jakobs, Philips CEO